


Hemopatch

SEALING HAEMOSTAT


Application Steps – as easy as 1, 2, 3...

HEMOPATCH is intended as a haemostatic device and surgical sealant for procedures in which control of bleeding or leakage of other body fluids or air by conventional surgical techniques is either ineffective or impractical. HEMOPATCH may be used to close dural defects following traumatic injury, excision, retraction or shrinkage of the dura mater.¹

HEMOPATCH comes ready to use in sterile packages and must be handled accordingly. Use only undamaged packages, single use only, do not re-sterilise.

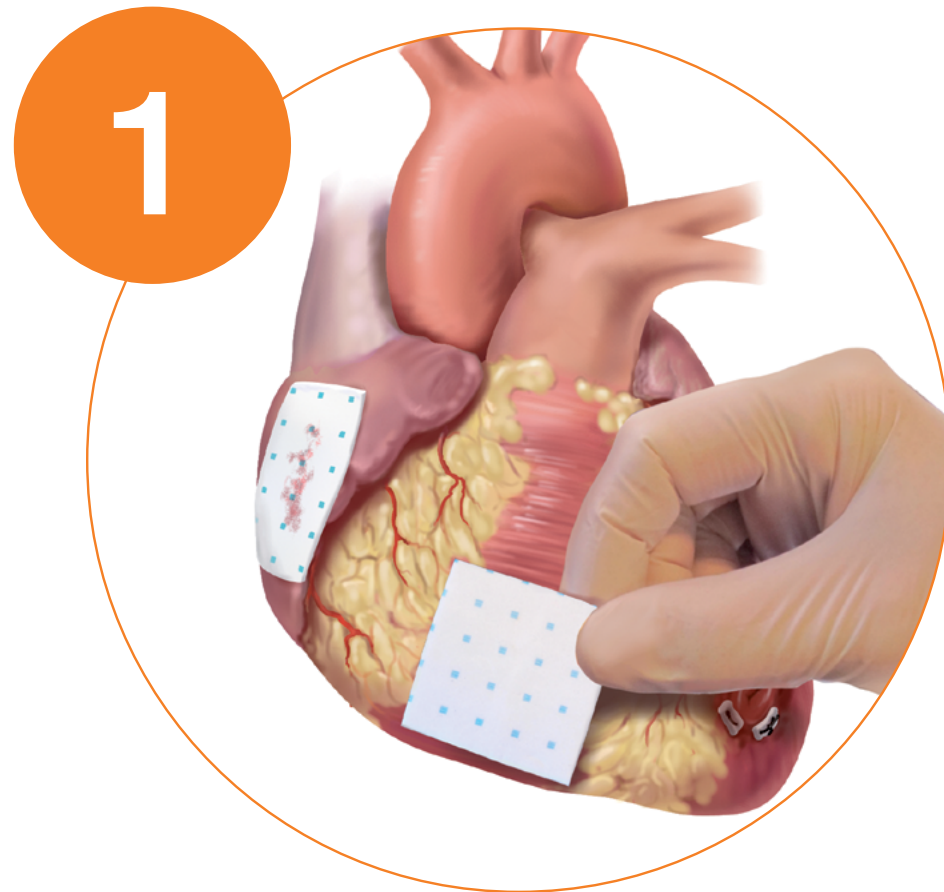


Apply HEMOPATCH **dry** with blue dots facing **up** and the white non-marked side in contact with the bleeding surface

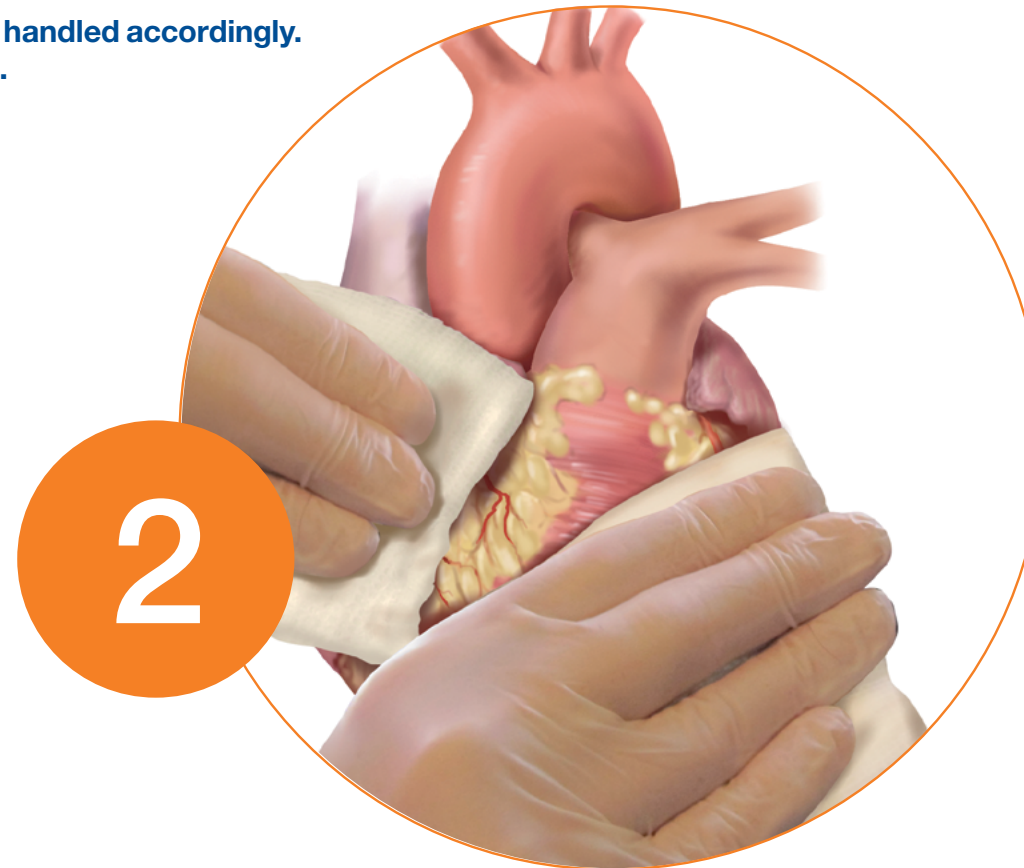

Use a **dry gauze** and approximate HEMOPATCH with gentle uniform pressure for 2 minutes

Improved adherence is observed when HEMOPATCH is in direct contact with wound fluid such as blood or lymphatic fluid

In the absence of such wound fluids, sodium bicarbonate solution (concentration between 4.2% to 8.4%) may be used in conjunction with HEMOPATCH application

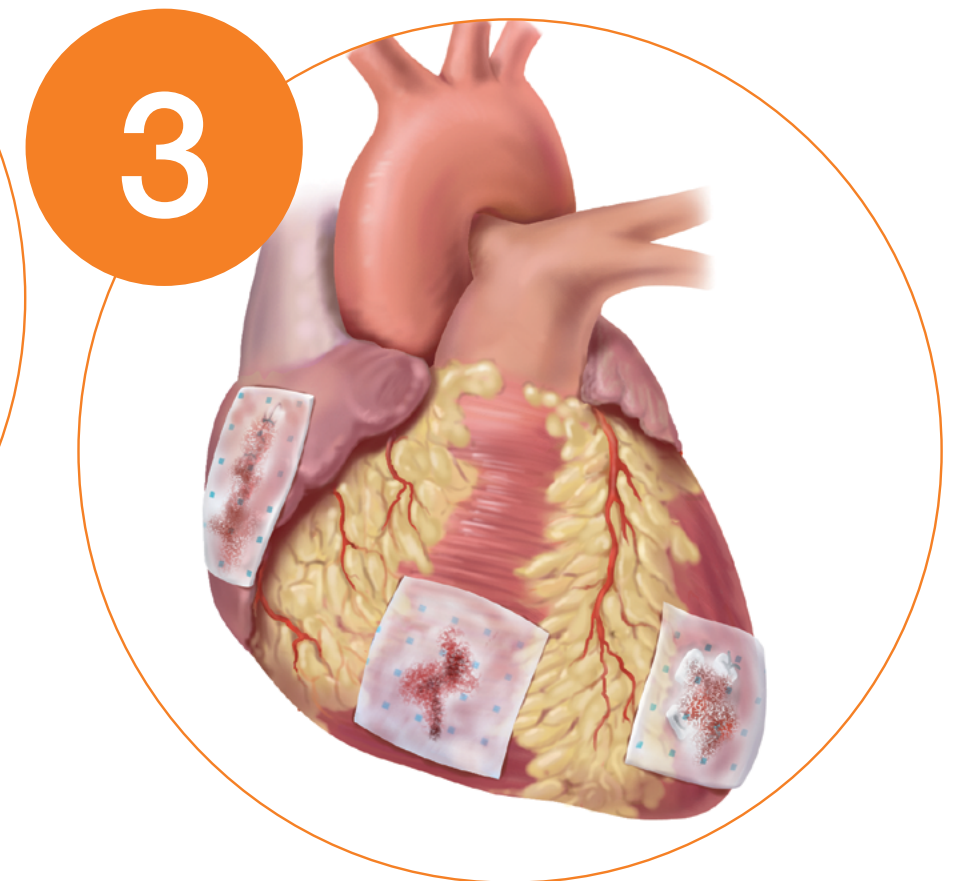

Confirm haemostasis has been achieved and leave HEMOPATCH in situ; **avoid disrupting the clot-formation**

Hemopatch

SEALING HAEMOSTAT

Ordering information	Size	Units per box	Order Number
HEMOPATCH Small	2.7 x 2.7 cm	5	1506257
HEMOPATCH Medium	4.5 x 4.5 cm	3	1506256
HEMOPATCH Large	4.5 x 9.0 cm	3	1506253

Any medical device product quality complaints (including medical device adverse incidents) relating to Baxter products can be reported directly to the Baxter Country Quality Assurance Team:

In the UK on +44 (0)1604 704603, or by email to UK_SHS_QA_Complaints@baxter.com.

In Ireland on +353 (0)1 2065500 or by email to shs_complaints_dublin@baxter.com

Alternatively please report directly to your Baxter Representative, who will take the details and forward to the Baxter Country Quality Assurance Team.

Medical device adverse incidents should also be reported:

In the UK to the MHRA. Reporting forms and information can be found at: www.mhra.gov.uk/safetyinformation/reportingsafetyproblems/index.htm .

In Ireland to the HPRA. Reporting forms and information can be found at: <http://www.hpra.ie/homepage/about-us/report-an-issue>

REFERENCES

1. HEMOPATCH Sealing Hemostat Instructions for Use. December 2018.

Baxter

Baxter Healthcare Ltd.
Wallingford Road, Compton,
Newbury, Berkshire,
RG20 7QW

Baxter Healthcare Ltd.
Unit 7, Deansgrange Business Park
Blackrock
Co Dublin

www.baxterhealthcare.co.uk

www.baxterhealthcare.ie



Baxter and Hemopatch are trademarks for Baxter International Inc., its subsidiaries or affiliates.

UKI-AS21-230026 May 2023